

Certificate of Analysis

Product Name: Mouse Fibronectin ELISA Kit


Catalog No.: AAA13502

Lot No.: E02a/2023N

>> Typical Data & Standard Curve

Results of a typical standard run of a Mouse Fibronectin ELISA Kit for lot # E02a/2023N are shown below. This standard curve was generated at our lab for demonstration purpose only.

X	pg/ml	0	156	312	625	1250	2500	5000	10,000
Y	OD450	0.175	0.234	0.286	0.372	0.576	0.916	1.424	2.139

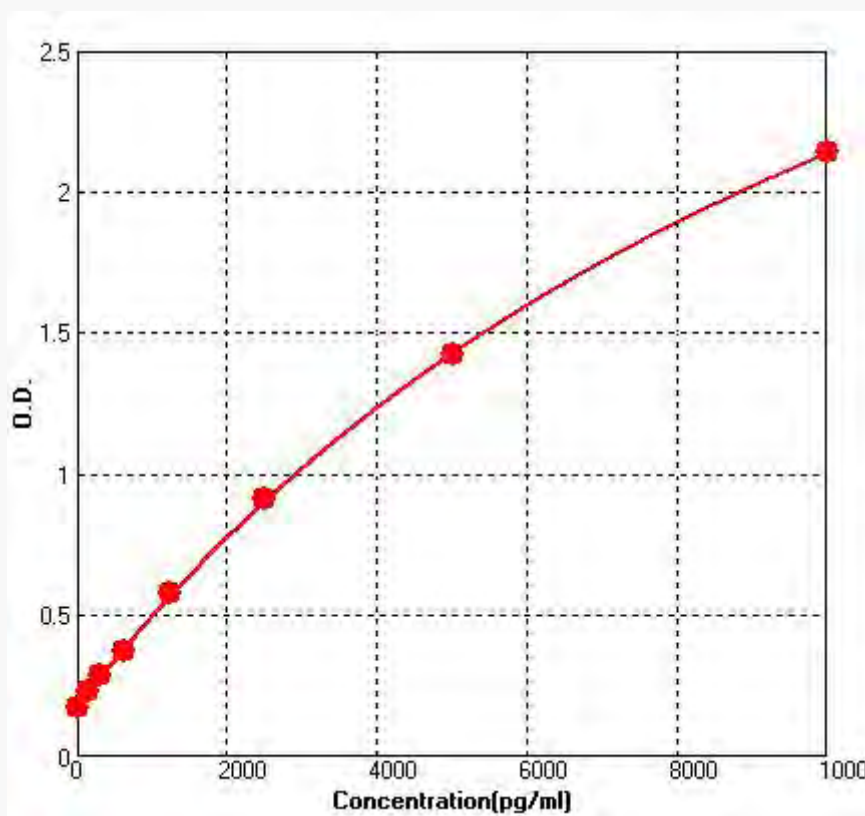

Remark: The standard curve was calculated by logistic 4PL.

>> Intra-Assay Precision

Three samples of known concentration were tested twenty times on one plate to assess intra-assay precision.

The %CV of intra-assay is < 10%

>> Inter-Assay Precision

Three samples of known concentration were tested in twenty separate assays to assess inter-assay precision.

The %CV of inter-assay is < 10%

>> Storage & Expiration

This kit can be stored at 2-8°C for 6 months, or at -20°C for 12 months. The manufacture date of this kit is November 02, 2023, so it can be effected until May 01, 2024 if store at 2-8°C, or November 01, 2024 if stored at -20°C.

Note: Avoid multiple freeze-thaw cycles.
