

Certificate of Analysis

Product Name: ELISA Kit for Toll Like Receptor 1 (TLR1)

Cat.No.AAA20341 Organism: Homo sapiens (Human)

Introduction

Item	Standard		Test Result
Description	This immunoassay kit allows for the specific measurement of TLR1 concentration in human tissue homogenates, cell lysates and other biological fluids.		Conform
Identification	Colorimetric		Positive
Composition	Pre-coated, ready to use 96-well strip plate Standard (freeze dried) Standard Diluent Detection Reagent A (green) Detection Reagent B (red) Assay Diluent A Assay Diluent B TMB Substrate Stop Solution Wash Buffer(30 x concentrate) Plate sealer for 96 wells Instruction manual	1 2 1 × 20ml 1 × 120µl 1 × 120µl 1 × 12ml 1 × 12ml 1 × 9ml 1 × 6ml 1 × 20ml 4 1	Conform
Assay Range	0.312-20ng/mL		Conform

Sensitivity


The minimum detectable dose of human TLR1 is typically less than 0.114ng/mL.

The sensitivity of this assay, or Lower Limit of Detection (LLD) was defined as the lowest protein concentration that could be differentiated from zero. It was determined the mean O.D. Value of 20 replicates of the zero standard added by their three standard deviations.

Standard curve

The standard curve is provided for demonstrated only. The client should perform the standard test in each independent experiment.

ng/ml	Standard		Average	Corrected
0	0.086	0.092	0.089	—
0.312	0.193	0.19	0.192	0.103
0.625	0.268	0.274	0.271	0.182
1.25	0.411	0.402	0.407	0.318
2.5	0.585	0.601	0.593	0.504
5	1.063	0.962	1.013	0.924
10	1.722	1.685	1.704	1.615
20	2.704	2.748	2.726	2.637

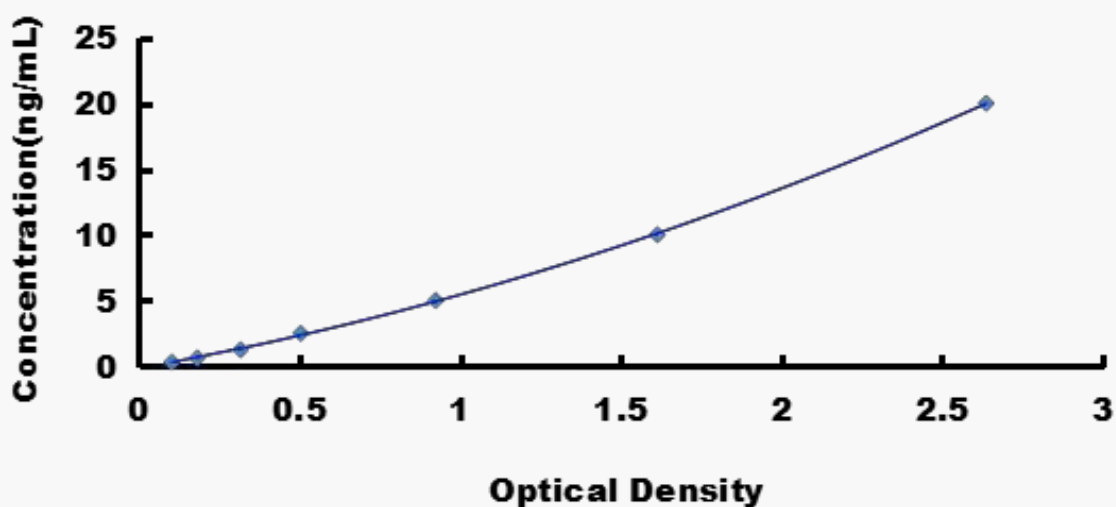

Precision

Intra-assay Precision (Precision within an assay): 3 samples with low, middle and high level of human TLR1 were tested 20 times on one plate, respectively.

Inter-assay Precision (Precision between assays): 3 samples with low, middle and high level of human TLR1 were tested on 3 different plates, 8 replicates in each plate.

Sample	Intra-assay Precision			Inter-assay Precision		
	1	2	3	1	2	3
n	20	20	20	24	24	24
Mean (ng/ml)	0.58	2.88	8.73	0.61	2.94	8.66
SD	0.042	0.192	0.542	0.046	0.202	0.565
CV (%)	7.2	6.7	6.2	7.5	6.9	6.5

Approved Date: 2017.1.19