

Certificate of Analysis

Spermine ELISA Kit

Cat.No.: AAA27612

Size: 96T


Lot: U2592I020

Principle: This ELISA kit uses Competitive-ELISA as the method

Product expiration Date: 2023/08/02

This product has been tested by Quality Control Department and meets performance specifications mentioned in the manual.

STD.(ng/ml)	OD-1	OD-2	Average
0	2.459	2.531	2.495
12.5	1.759	1.811	1.785
25	1.291	1.329	1.31
50	0.958	0.986	0.972
100	0.651	0.669	0.66
200	0.427	0.439	0.433
400	0.225	0.231	0.228
800	0.111	0.115	0.113

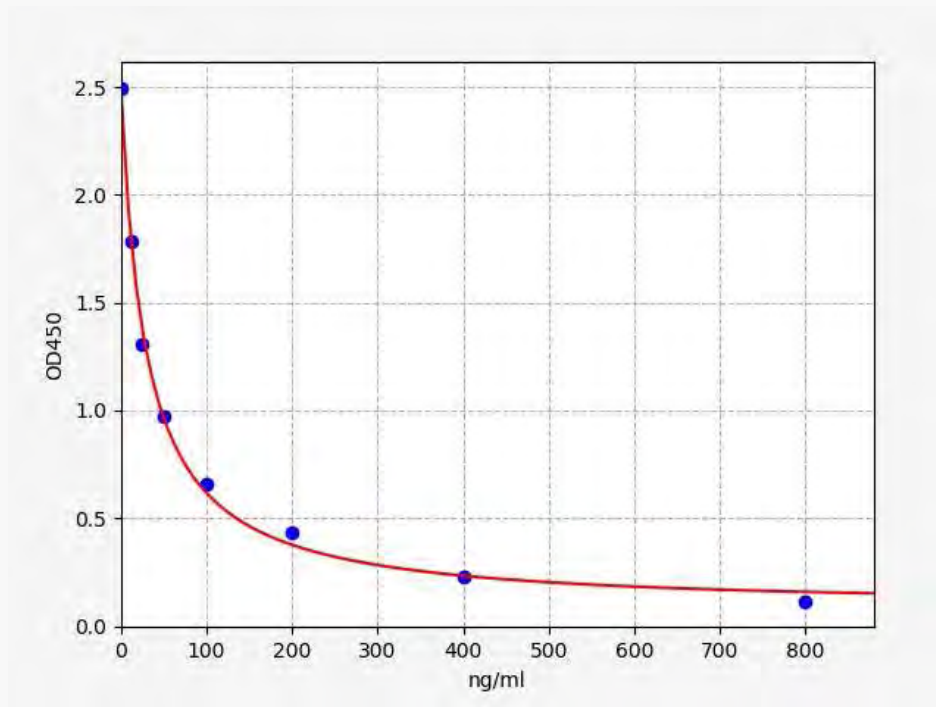

Performance Characteristics

Intra-Assay CV: <8%

Inter-Assay CV: <10%

Manufacture date: 2023/02/02