

## Certificate of Analysis

### PRODUCT INFORMATION

**Catalog Number:**AAA27887

**Product Name:** Proline Microplate Assay Kit

**Lot Number:** CM1E21A

### COMPONENTS

Component	Quantity	Result
96-Well Microplate	1 plate	Pass
Assay Buffer	30 ml x 4	Pass
Reaction Buffer	5 ml x 1	Pass
Dye Reagent	Powder x 1	Pass
Dye Reagent Diluent	5 ml x 1	Pass
Standard	Powder x 1	Pass
Plate Adhesive Strips	3 Strips	Pass


### ASSAY

Reagent	Sample	Standard	Blank
Sample	50 µl	--	--
Standard	--	50 µl	--
Distilled water	--	--	50 µl
Reaction Buffer	50 µl	50 µl	50 µl
Dye Reagent	50 µl	50 µl	50 µl

Mix, put it into the convection oven, 90 °C for 20 minutes, mix, record absorbance measured at 520 nm.

### RESULT

for research use only

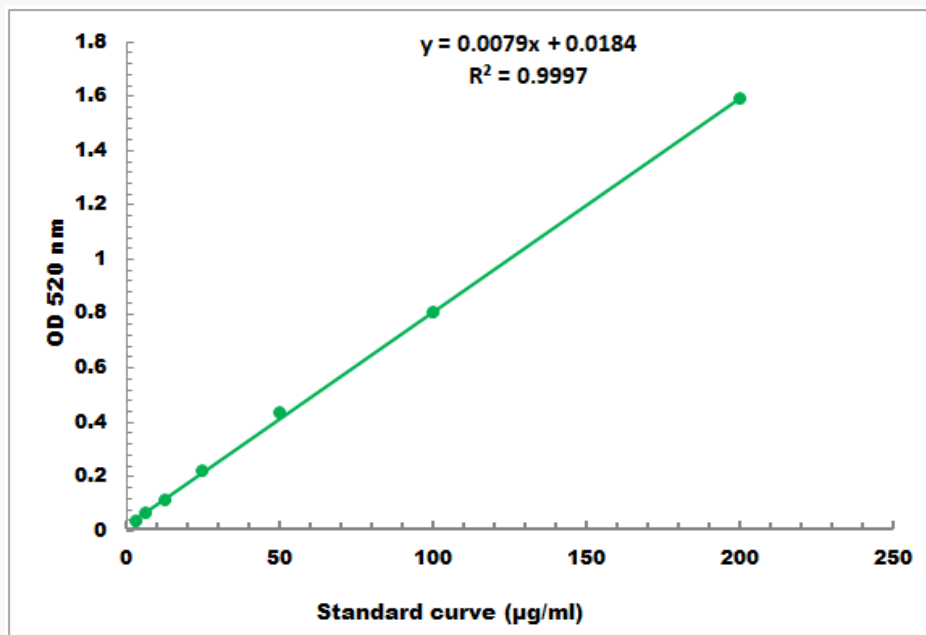

This product was tested and conformed to Assay kit's quality standard.